

## Larident Srl


Via Lamaneigra, 12 r (Ponte Rimassa) - 16030 Tribogna Genova

Tel. +39 0185 939 481 - Fax +0185 938 595

info@larident.it - www.larident.it

**LARIDENT**

MADE IN ITALY  
SINCE 1985

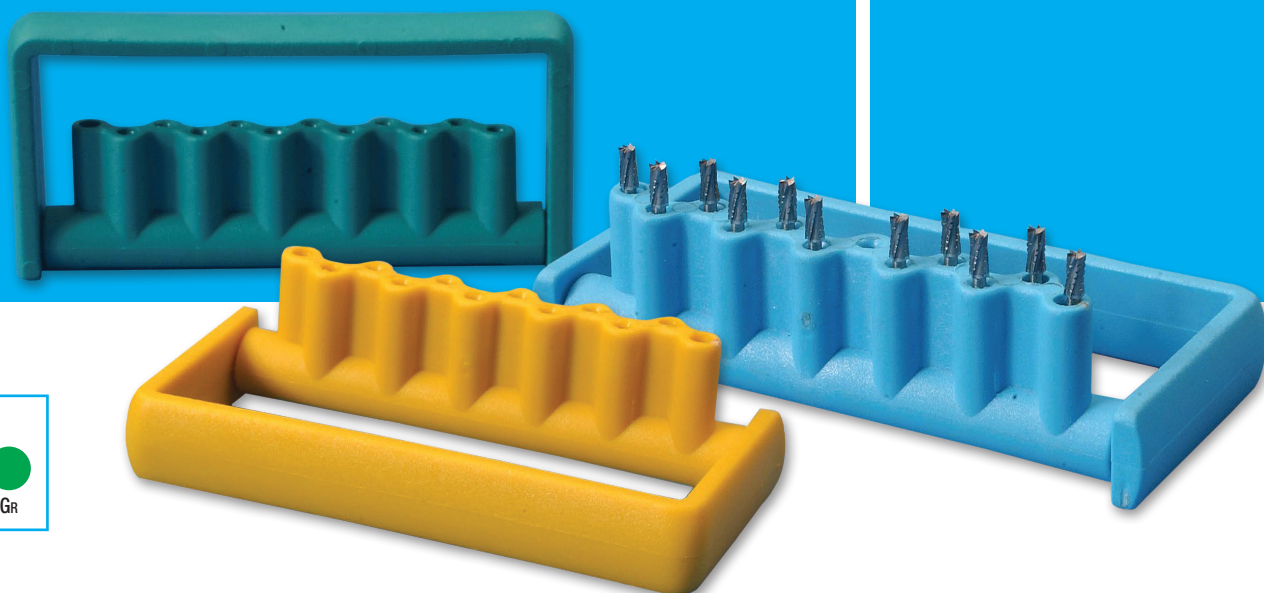

### AVAILABLE COLORS



Lb

Ye

Gr

# TECHNICAL DATA SHEET

PRODUCT NAME	Click-lock burs holder
ITEM CODE	L84
MATERIAL/COMPONENTS	Polyamide
THERMAL PROPERTIES	Autoclavable up to 121°C
MECHANICAL AND PHYSICAL CHARACTERISTICS	<ul style="list-style-type: none"><li>• Snap-on burs holder with 4 large holes RA/HP and 8 small holes FG for ultrasonic cleaning</li><li>• Available in: blue, yellow and green</li><li>• Measures: 7,5x3,5x12 cm</li></ul>
CLEANING	Use a cleaning agent suitable for the material
SAFETY DATA SHEET	N/N
INSTRUCTIONS FOR USE	This product is for professional use only
PRECAUTIONS/WARNINGS	Non-sterile
DISPOSAL	Disposal of the product must comply with local regulations and environmental guidelines
CLASSIFICATION REGULATION UE 2017/745	Not a medical device
RISKS ANALYSIS IN REF. D.L. 46 24/2/97	N/A

N/A = NOT APPLICABLE

N/N = NOT NECESSARY

## Larident Srl


Via Lamaneigra, 12 r (Ponte Rimassa) - 16030 Tribogna Genova

Tel. +39 0185 939 481 - Fax +0185 938 595

info@larident.it - www.larident.it

**LARIDENT**

MADE IN ITALY  
SINCE 1985

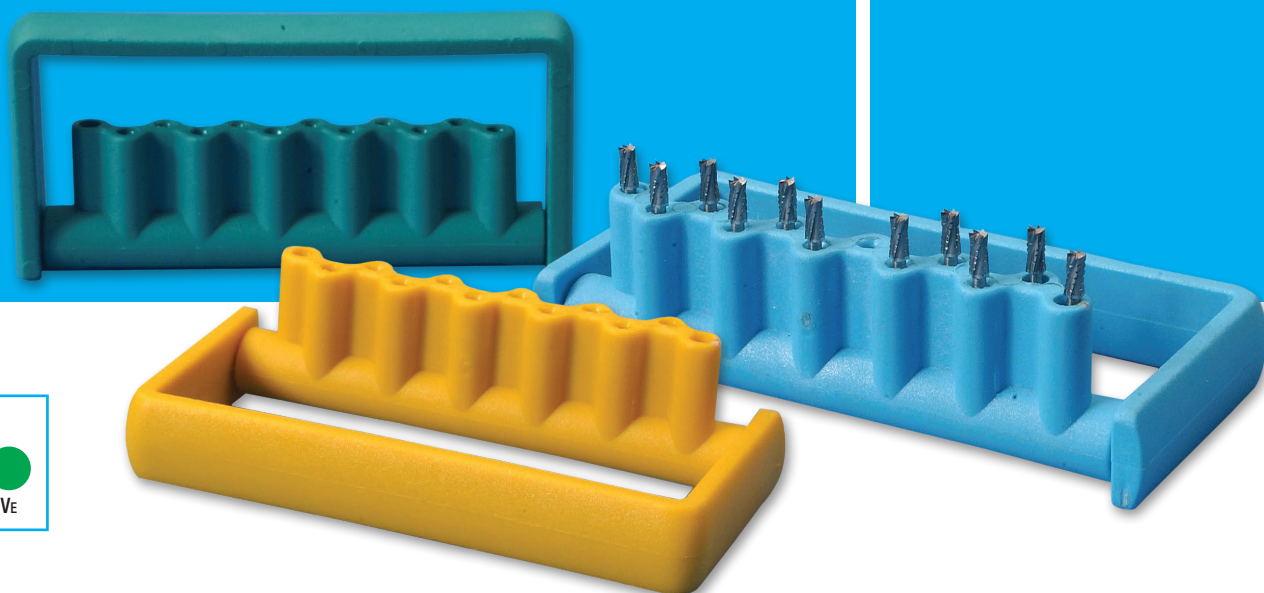

### GAMMA COLORI



# SCHEDA TECNICA DEL PRODOTTO

PRODOTTO	Portafrese a scatto
NS CODICE	L84
MATERIALE	Poliammide
PROPRIETÀ TERMICHE	Autoclavabile a 121°C
PROPRIETÀ MECCANICHE, FISICHE E CARATTERISTICHE	<ul style="list-style-type: none"><li>• Portafrese a scatto con 4 fori grandi RA/HP e 8 fori piccoli FG per pulizia a ultrasuoni</li><li>• Disponibile nei colori: azzurro, giallo e verde</li><li>• Misure: 7,5x3,5x12 cm</li></ul>
PULIZIA	Utilizzare solamente detergenti adatti al materiale
SCHEDA DI SICUREZZA	N/N
ISTRUZIONI PER L'UTILIZZO	Destinato esclusivamente a uso professionale
PRECAUZIONI	Non sterile
SMALTIMENTO	Lo smaltimento del prodotto deve essere conforme alle normative ed alle linee guida ambientali locali
CLASSIFICAZIONE REGOLAMENTO UE 2017/745	Non è un dispositivo medico
ANALISI DEI RISCHI IN RIF. D. L.46 24/2/97	N/A

N/A = NON APPLICABILE

N/N = NON NECESSARIA